


Test date: 2024-12-27,9:54:39

Tester: zhu zhifang
Report time : 2024-12-27,10:46:39
Method :Area Normalization Method

Instrument type:gas chromatography detector:FID

sample injector:distributary column temperature:temperature programming

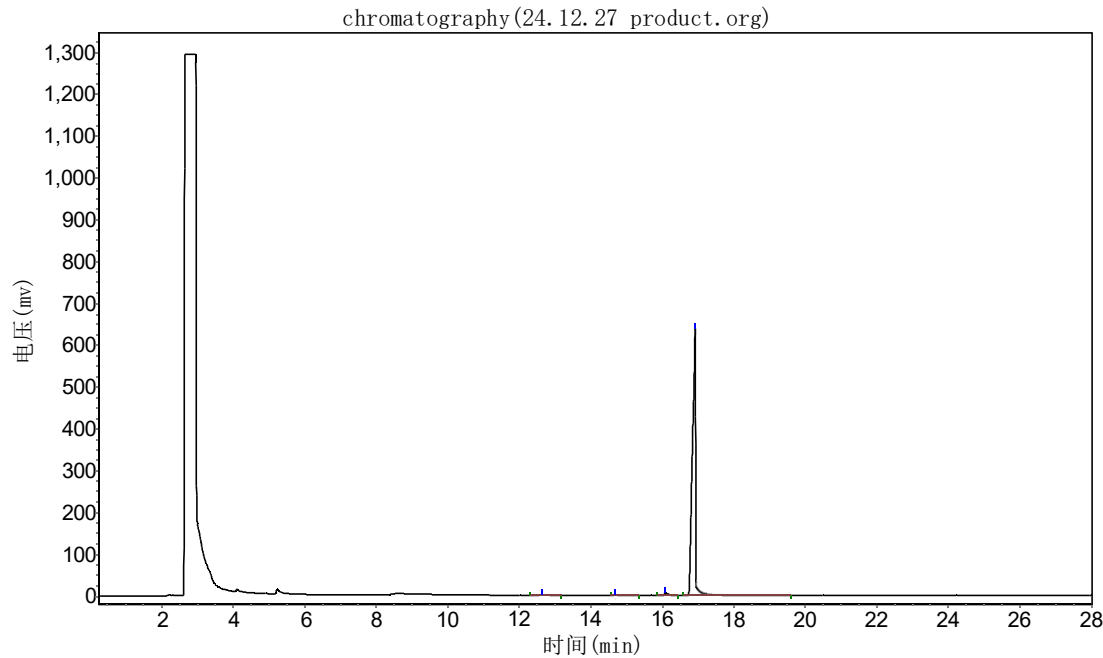

Analysis result table

Peak no.	Peak name	retention time	peak height	peak area	content
1		12.632	1283.436	17649.299	0.4204
2		14.675	2132.705	15872.604	0.3781
3		16.087	6795.339	46546.797	1.1088
4		16.920	637744.313	4117757.500	98.0926
Total			647955.793	4197826.199	100.0000