

File D:\DATA\20260609000007.D

Injection Date : 9 Jun 26 9:38 am +0800

Tgt Mass(EZX) :

Sample Name : XL029-013-2

Location : Vial 23

Acq. Operator :

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : C:\CHEM32\1\METHODS\TEST254-50-12.M

Analysis Method : D:\DATA\20260609000007.D\DA.M

Sample Info :


Method Info : Mobile phase: A: 0.1%TFA Water B: 0.1%TFA ACN

Gradient:


Flow Rate: 1.8ml/min

Column Temperature: 45 C

VWD1 A, Wavelength=254 nm

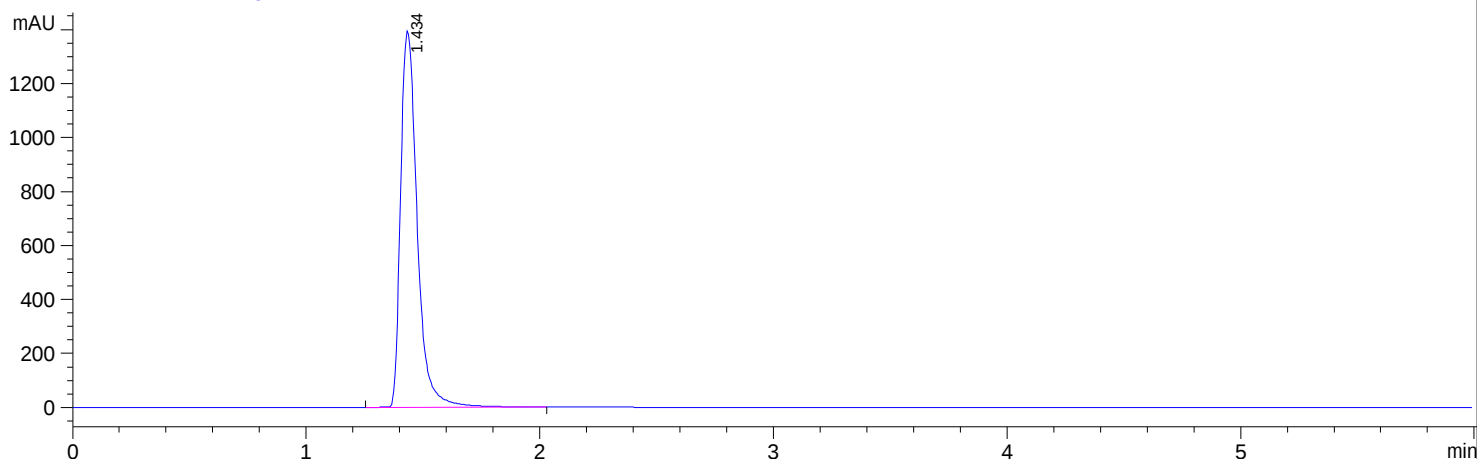


MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 100

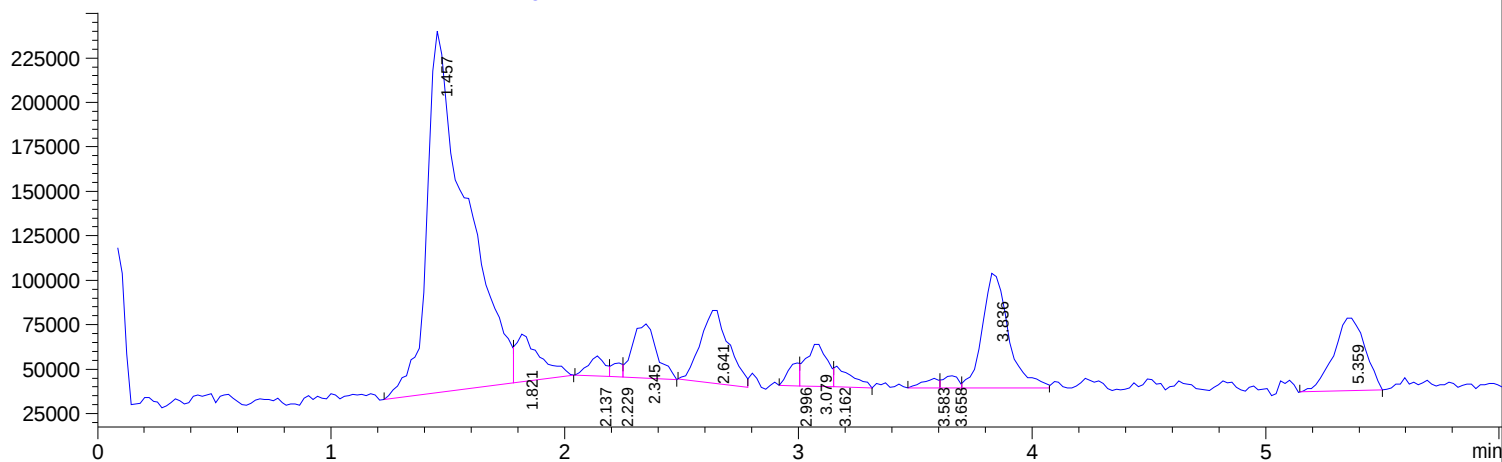


Integration Results for VWD1 A, Wavelength=254 nm

RetTim	Width	Area	Height	Area%
1.43	0.08	6899.88	1394.20	100.00


Ret. Time: 1.46 <<<< POSITIVE SPECTRA >>>>

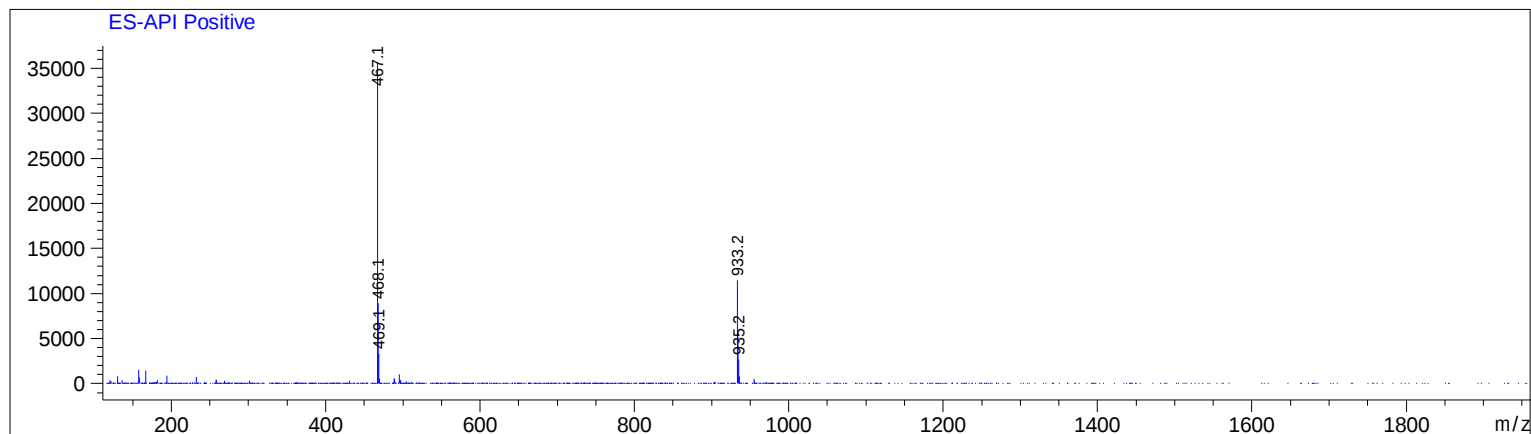


Ret. Time: 1.82

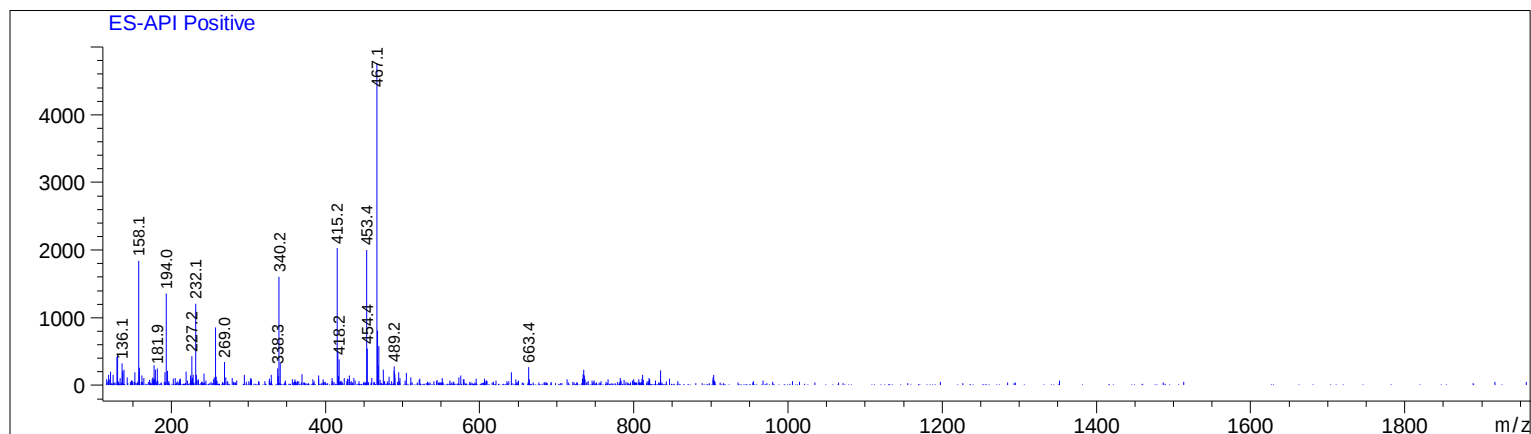


Ret. Time: 2.14

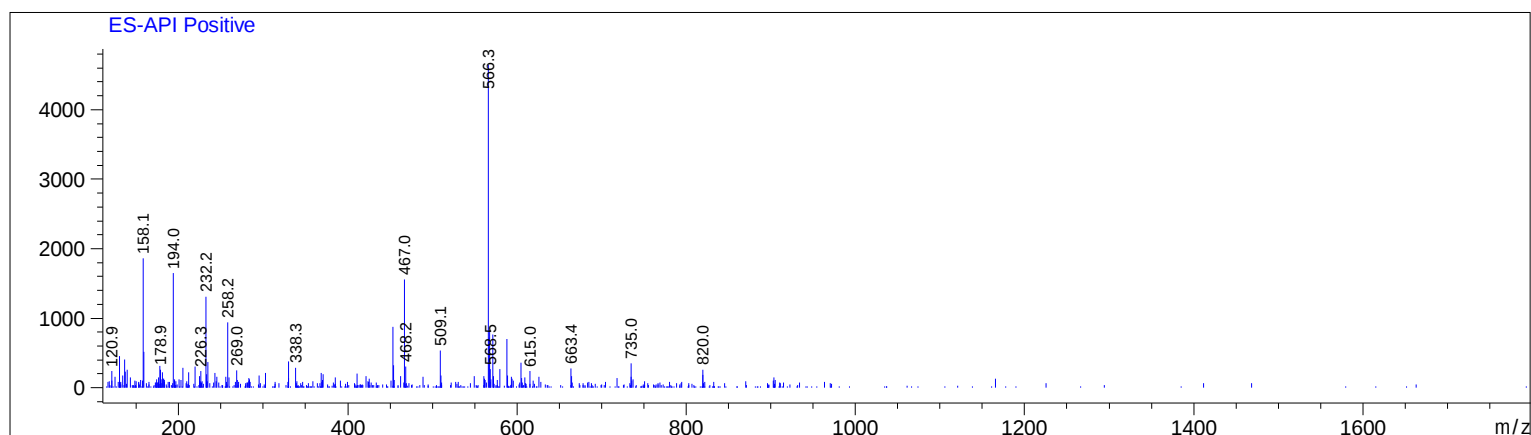


Ret. Time: 2.23

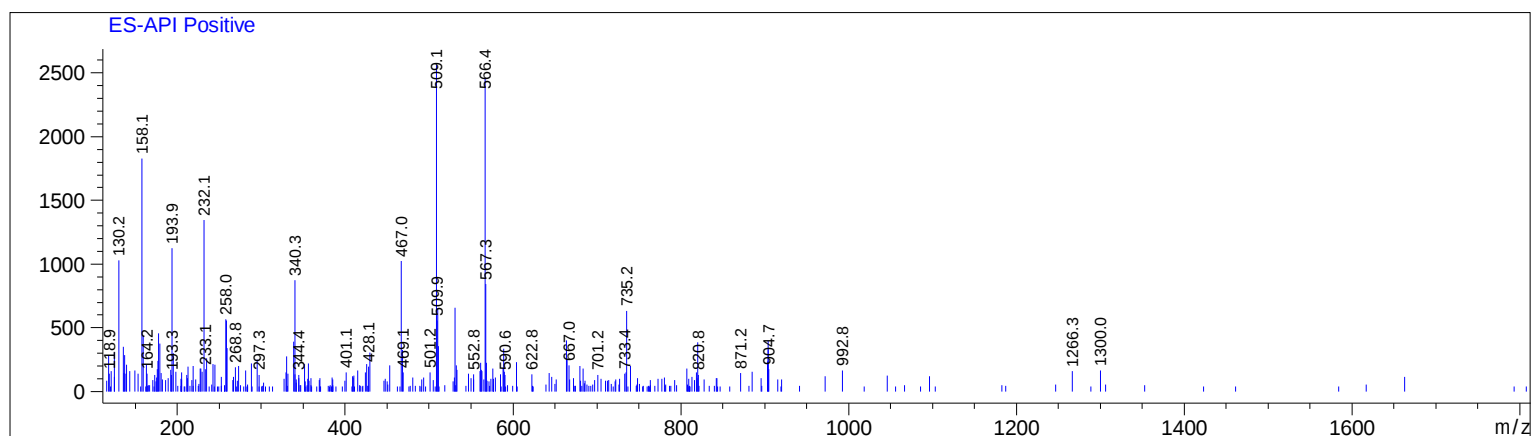


Ret. Time: 2.35

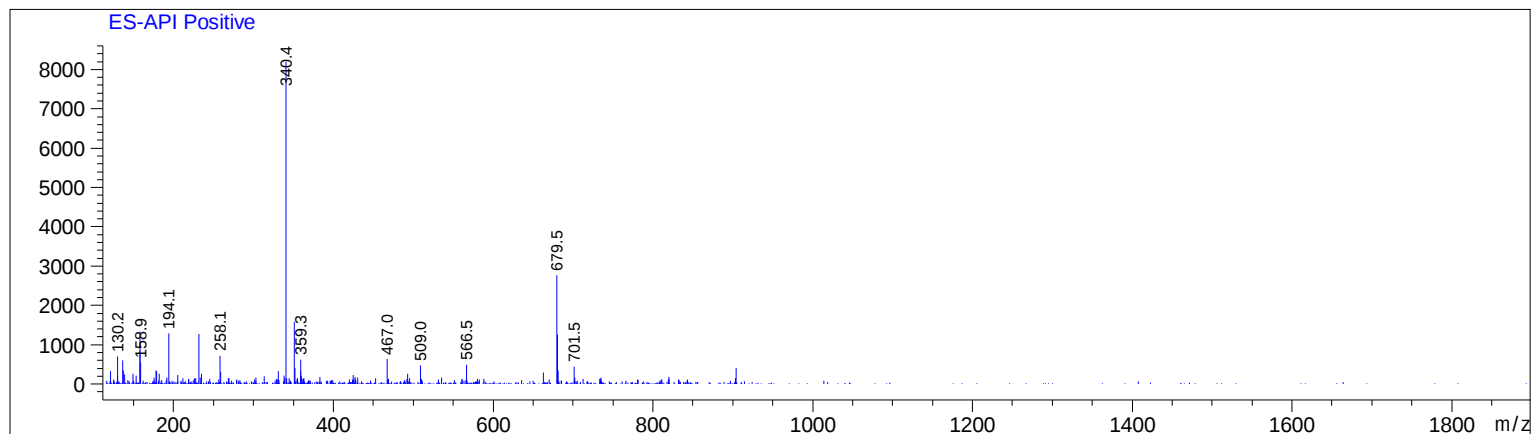


Ret. Time: 2.64

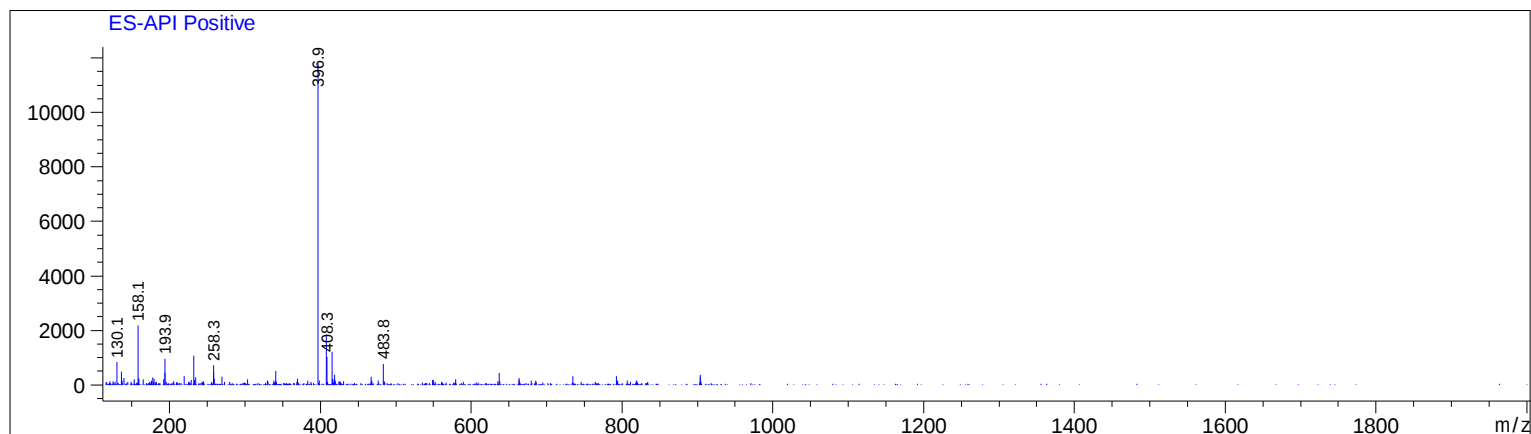


Ret. Time: 3.00

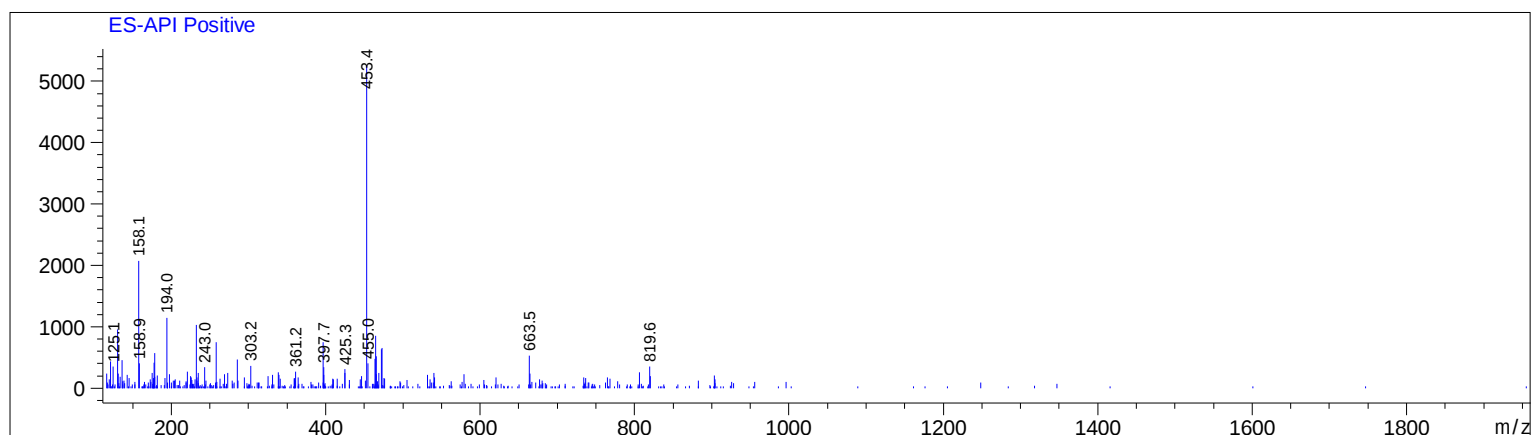


Ret. Time: 3.08

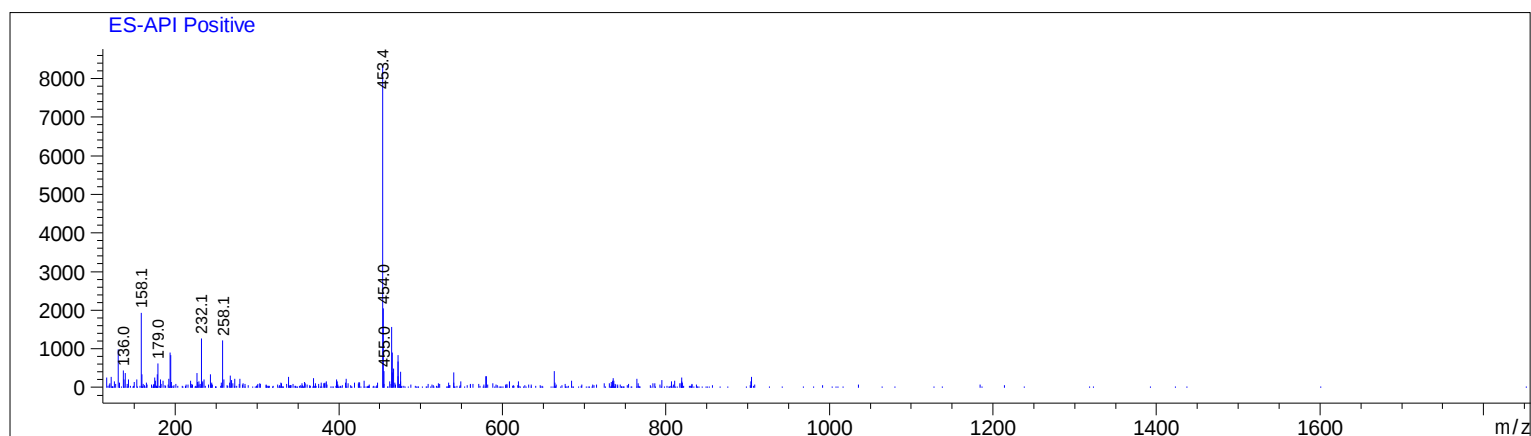


Ret. Time: 3.16

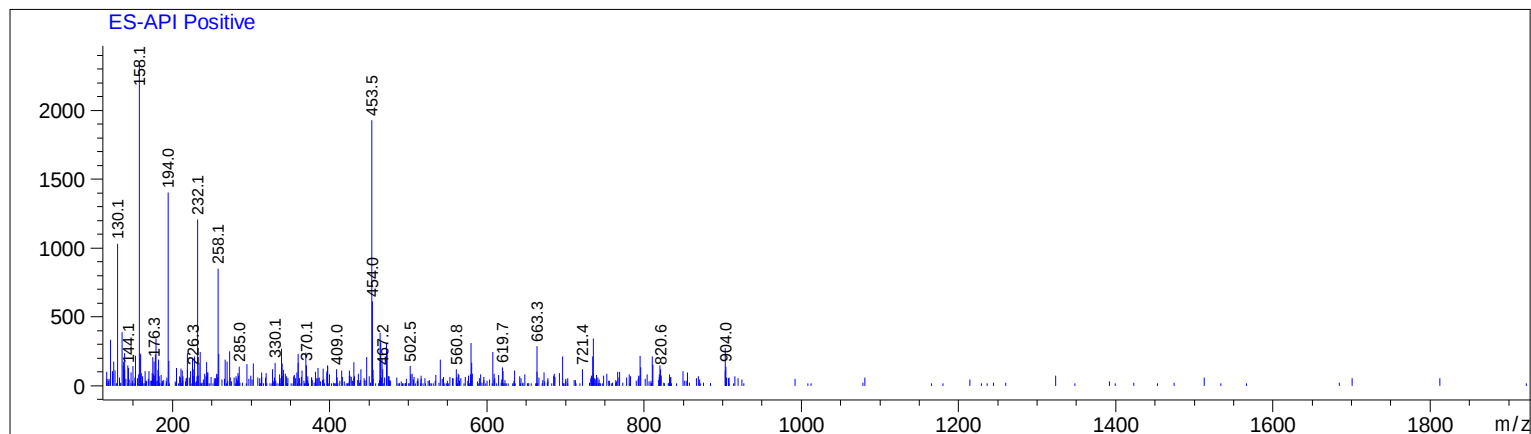


Ret. Time: 3.58

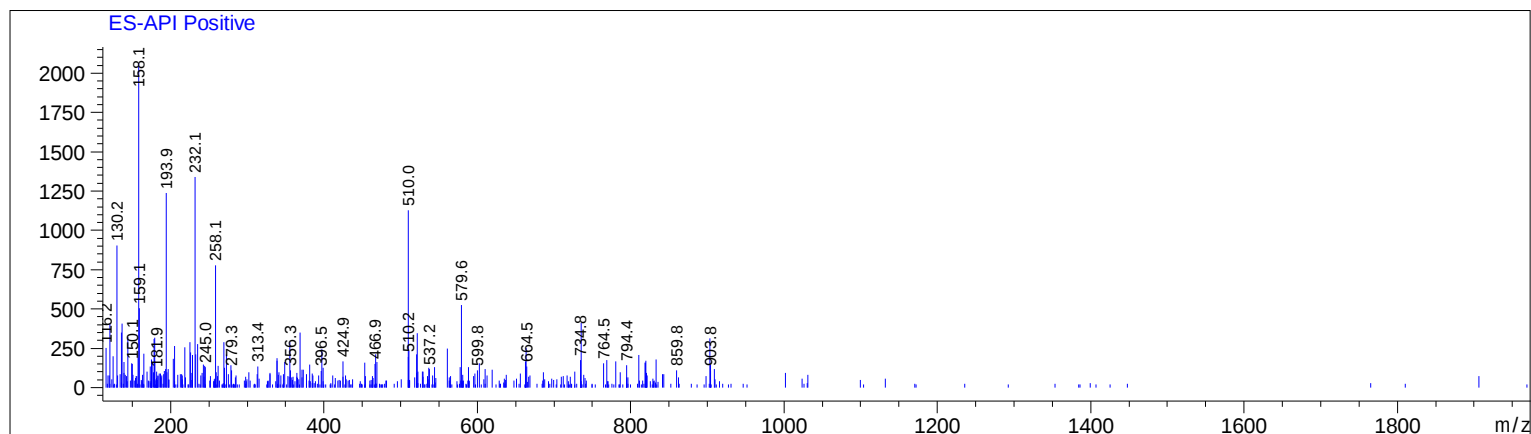

Ret. Time: 3.66

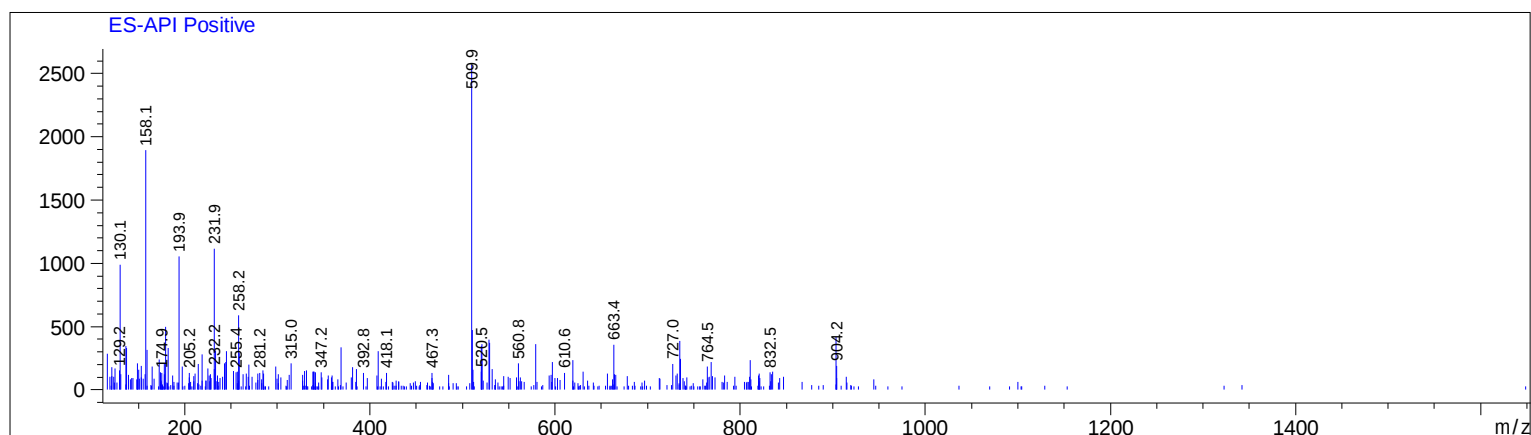

Ret. Time: 3.84

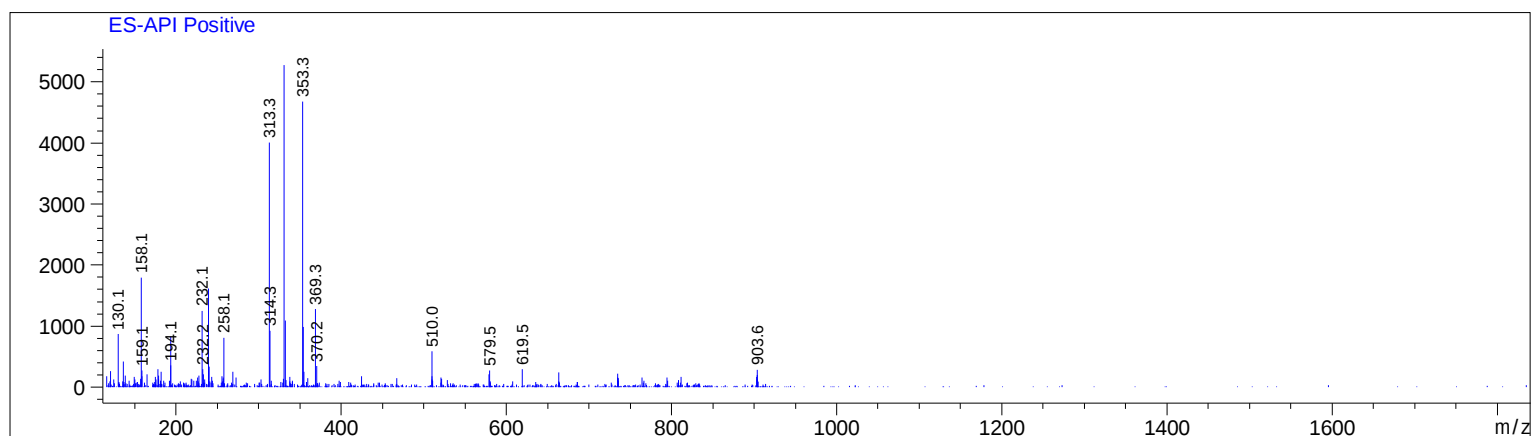

Ret. Time: 5.36

